




GUIDED


PYLON SURGICAL DRILLING PROTOCOL

Implant Ø 5.0 x 10.0mm

Guide Sleeve Offset 9.5

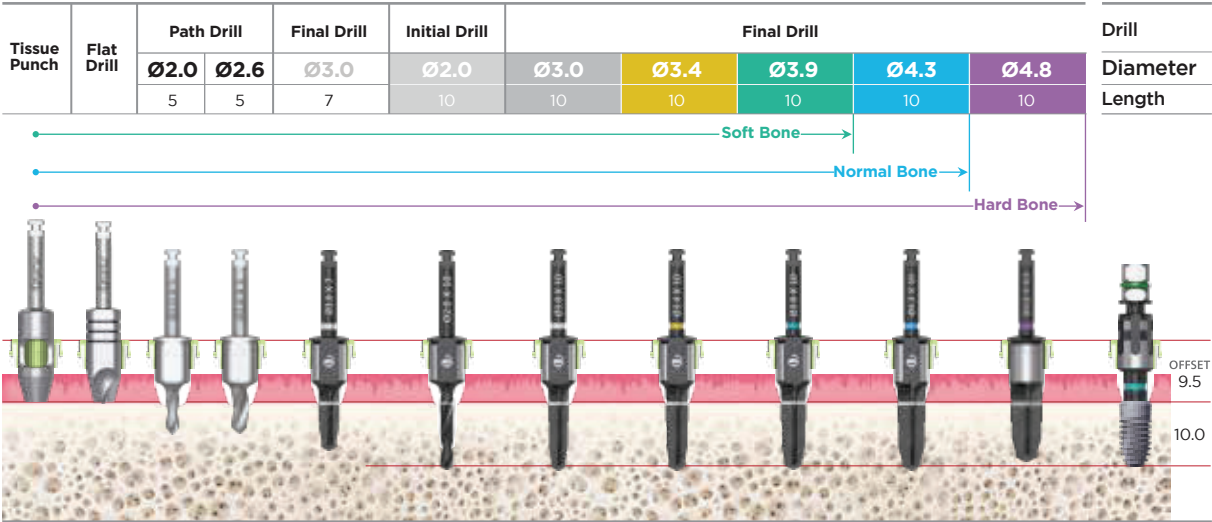

Guide Sleeve Offset 11.0

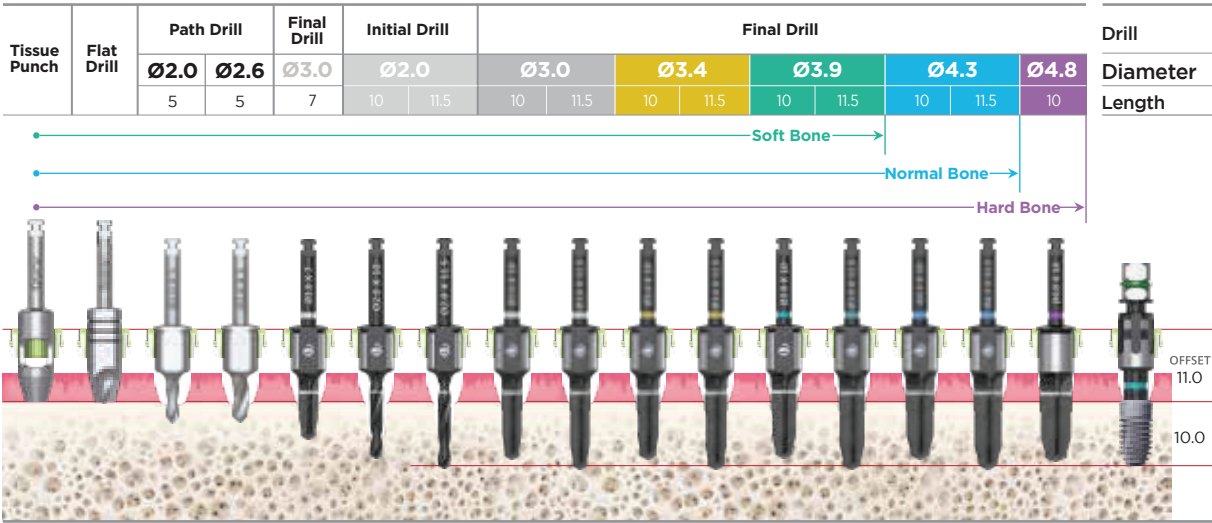

Implant Ø 5.0 x 10.0mm

Guide Sleeve Offset 12.5

